

OVERVIEW

Included with the MSO-3M cable shipment are the following:

- Qty 1 - 18 channel 3M connector cable
- Qty 1 – MSO-3M Instruction sheet (this document)

OPERATING ENVIRONMENT

Before using the MSO-3M cable, ensure that its operating environment will be maintained within these parameters:

Temperature:	5 to 40 °C
Humidity:	≤ 80% RH (non-condensing)

SAFETY REQUIREMENTS



CAUTION

To avoid personal injury or damage to the MSO-3M or any equipment connected to it, review and comply with the following safety precautions.

- **Use only as intended.** The MSO-3M cable is intended to be used only with LeCroy MS-250, MS-500 or MS-500-36 Mixed Signal Oscilloscope options. Use of the MSO-3M and/or the equipment it is connected to in a manner other than specified may impair the protection mechanisms.
- **Connect and disconnect properly.** Avoid damage to cables thru excessive bending. When disconnecting the MSO-3M cable from the MS-250, MS-500, MS-500-36 or Device Under Test NEVER pull on the blue wires, pull only the black plastic housing.
- **Do not use in wet/damp or explosive atmospheres.**
- **For indoor use only.** The MSO-3M cable and associated test equipment is intended for indoor use and should be operated in a clean, dry, environment.
- **Do not operate with suspected failures.** Do not use the product if any part is damaged. All maintenance should be referred to qualified service personnel.

BASIC OPERATION

Connecting the MSO-3M to the MS-250 or MS-500

- Connect the end of the cable labeled D0 – D17 to the corresponding input of the MS-250 or MS-500 labeled D0 – D17 and fasten thumb screws

Note: MS-500 can be operated in 36 channel mode by using two MS-3M cables however both MSO-3M cables will be labeled D0-D17.

Connecting the MSO-3M to the Device Under Test

- The MSO-3M cable mates with the following 3M Through-Hole 2500 series connectors

2520-6002 (straight)
2520-5002 (right-angle)


Looking into the 3M Connector:

Connector Pin #	1	3	5	7	9	11	13	15	17	19
	NC	D16	D14	D12	D10	D8	D6	D4	D2	D0
	D17	D15	D13	D11	D9	D7	D5	D3	D1	Gnd
Connector Pin #	2	4	6	8	10	12	14	16	18	20

SPECIFICATIONS

Input Impedance	100 k Ω
Attenuation	10:1
Maximum Input Voltage	$\leq 30 V_{pk}$

All specifications are for the MSO-3M cable used with the MS-250, MS-500 or MS-500-36

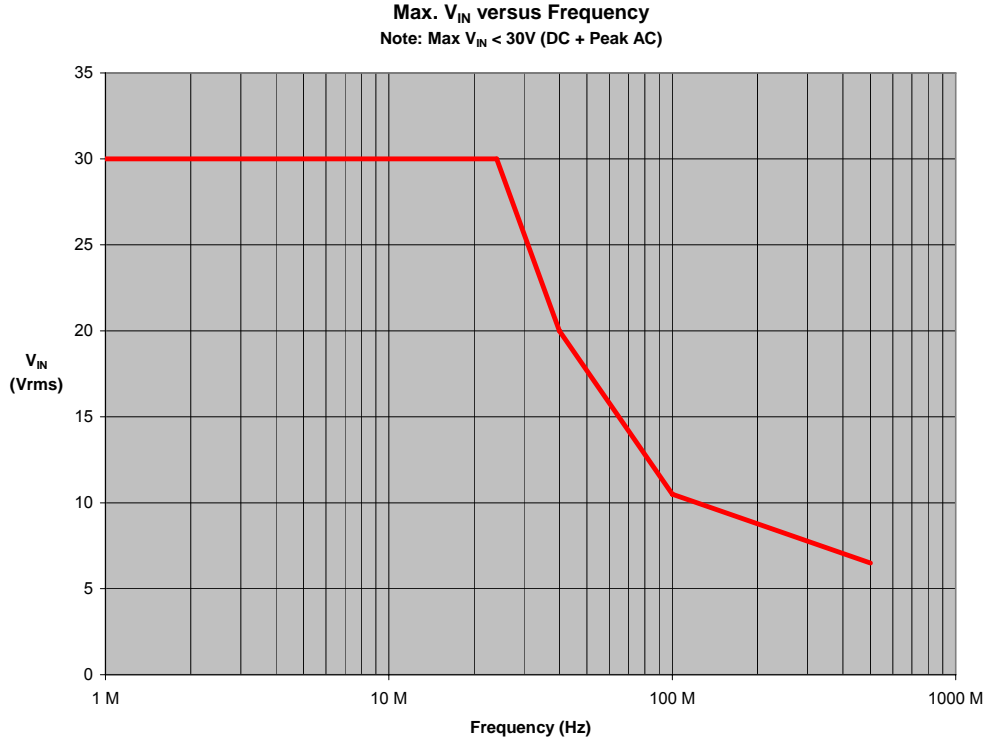

X-ON Electronics

Largest Supplier of Electrical and Electronic Components

Click to view similar products for [Benchtop Oscilloscopes](#) category:

Click to view products by [Teledyne](#) manufacturer:

Other Similar products are found below :

[WSXS-RACK](#) [WSXS-MOUSE](#) [WSXS-KYBD](#) [UPO2102CS](#) [AX-DS1100CFM](#) [TT-HV250](#) [TT-LF212](#) [TT-LF 312-2-6](#) [DSO3064-KIT-IV](#)
[DSO5102P](#) [DSO5202B](#) [RT-ZP03](#) [MSO5062D](#) [CC-650](#) [FLUKE PM9082/001](#) [TOS-2020CT](#) [PK007-003](#) [PK007-019](#) [PK007-022](#) [PK007-024](#)
[PK007-026](#) [PK106-5](#) [PK116-3](#) [PK1-5MM-102](#) [PK1-5MM-104](#) [PK1-5MM-105](#) [PK1-5MM-108](#) [PK1-5MM-111](#) [PK1-5MM-112](#) [PK1-5MM-](#)
[113](#) [PK1-5MM-120](#) [TA041](#) [GDS-1052-U](#) [GDS-1072A-U](#) [GDS-1102A-U](#) [GDS-2072A](#) [GDS-2202E](#) [GDS-2204E](#) [U3400A-1CM](#) [PP-150](#) [PP-](#)
[80](#) [HO720](#) [TT-MF312](#) [TT-LF316](#) [TT-HV150](#) [TT-HF212RA](#) [TT-HF212](#) [2555](#) [2557](#) [2566](#)