



## testo • Smart Probes

Startup instruction

---



# 1 Safety

## 1.1. Safety with testo 510i

**⚠ WARNING**  
Magnetic field  
**May be harmful to those with pacemakers.**  
> Keep a minimum distance of 10 cm between pacemaker and instrument.

## 1.2. Safety with testo 549i

**⚠ WARNING**  
Risk of injury caused by pressurized, hot, cold or toxic refrigerants/media!  
> Only to be used by qualified staff.  
> Wear protective goggles and safety gloves.  
> Before applying pressure to the measuring instrument: always fix the instrument tightly onto the pressure connection.  
> Comply with the permissible measuring range (0 to 60 bar). Pay particular attention to this in systems with R744 refrigerant, since these are frequently operated with higher pressures!

## 1.3. Safety with testo 805i

**⚠ CAUTION**  
**Laser radiation! Class 2 laser**  
> Do not look into the laser beam!


# 2 Overview



- 1 Measuring unit
- 2 LED
- 3 Key
- 4 Battery compartment (at the back)

## 3 Switching on/off

### 3.1. Switching on

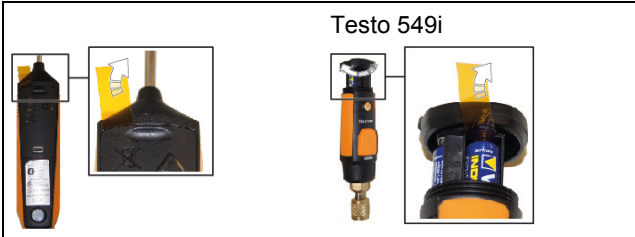

1. Pull the film out of the battery compartment.
2. Press the key.
  - The Smart Probes switch on.

### 3.2. Switching off

1. Press and hold the key.
  - The Smart Probes switch off.

## 4 Bluetooth® module

### 4.1. Establishing Bluetooth® connection



You need a Tablet or Smartphone with the Testo Smart Probes App already installed on it to be able to establish a Bluetooth connection.

You can get the App for iOS instruments in the App Store or for Android instruments in the Play Store.

Compatibility:

- requires iOS 8.3 or later / Android 4.3 or later
- requires Bluetooth 4.0

### 4.2. Bluetooth® approval



The Bluetooth® option may only be operated in countries in which it is type approved. For further information, please refer to the instruction manual at: [www.testo.com/smartprobesmanuals](http://www.testo.com/smartprobesmanuals).

FCC (Federal Communications Commission) countries information

This instrument complies with part 15 of the FCC Rules. Its commissioning is subject to the following two conditions: (1) This instrument must not cause any harmful interference and (2) this instrument must be able to accept interference, even if this could have undesired effects on operation.

Changes

The FCC demands that the user be informed that any changes or modifications to the instrument that have not been explicitly approved by Testo AG may void the user's right to use this instrument.

To find out how to handle the product safely and for detailed information, please refer to the instruction manual at: [www.testo.com/smartprobesmanuals](http://www.testo.com/smartprobesmanuals).

## 5 LED status

LED status	Meaning
Flashing red	Low battery status
Flashing yellow	<ul style="list-style-type: none"><li>• Smart Probe is switched on.</li><li>• Smart Probe searching, but not yet connected.</li></ul>
Flashing green	<ul style="list-style-type: none"><li>• Smart Probe is switched on.</li><li>• Bluetooth is connected.</li></ul>

## 6 Transmitting reading

- ✓ The Smart Probes are switched on and connected to their mobile terminal via Bluetooth.
1. The Smart Probes' readings are automatically shown in the standard display.
  2. Press the key.
    - The reading that is currently present is held.
  3. Press the key again.
    - The instrument again displays the current readings.



These commissioning instructions describe the basic operating steps.

To find out how to handle the product safely and for detailed information, please refer to the instruction manual at:  
[www.testo.com/smartprobesmanuals](http://www.testo.com/smartprobesmanuals).

---

## X-ON Electronics

Largest Supplier of Electrical and Electronic Components

*Click to view similar products for [Testo manufacturer:](#)*

Other Similar products are found below :

[206 PH1](#) [TESTO 316-1 0632 0316](#) [TESTO 470 0563 0470](#) [TESTO 770-1 0590 7701](#) [TESTO 905-T1 0560 9055](#) [0572 0500](#) [0590 0016](#) [0602 4592](#) [0590 0008](#) [0590 0018](#) [0602 0645](#) [0635 1025](#) [0628 0020](#) [TESTO 435-2 0563 4352](#) [TESTO 605I 0560 1605](#) [TESTO 755-2 0590 7552](#) [TESTO 770-2 0590 7702](#) [TESTO 869 + TESTO 745](#) [TESTO 869 + TESTO 750-3 465 410-2 460 0572 6172 0590 0001 0614 2272](#) [TESTO 417 0560 4170](#) [0609 7072](#) [TESTO 174-H SET](#) [TESTO 176-T4](#) [TESTO 176-P1](#) [TESTO 830-T2](#) [TESTO 103](#) [TESTO 905-T1](#) [TESTO 108-2](#) [TESTO 905I](#) [TESTO 108 0563 4403](#) [0590 7703](#) [TESTO 435-3 0560 4353](#) [TESTO 735-1 0560 7351](#) [TESTO 760-3 0590 7603](#) [TESTO 770-3 0590 7703](#) [0590 0013](#) [0602 4892](#) [TESTO 635-2 0563 6352](#) [TESTO 750-3 0590 7503](#) [TESTO 760-1 0590 7601](#) [816-1](#) [TESTO 174-T SET](#) [TESTO 605-H1](#)