

# EL-GFX-1

## Temperature Data Logger with Graphic LCD Screen

### ORDERING INFORMATION

Standard Data Logger EL-GFX-1  
(Data Logger, 2 x Batteries, USB cover, Mounting Clip, Micro USB cable)


Replacement Battery BAT 3V6 ½AA  
(2 Required)

### FEATURES

- Rugged and robust IP67 construction
- -30 to +80 °C (-22 to +176 °F) measurement range
- Logging rates between 10 seconds and 1 hour
- Stores over 250,000 readings
- On screen menu and graphing to start, stop, review and restart the logger in the field
- Micro USB interface for PC based set-up and data download
- Immediate, delayed, push-button or temperature triggered start mode
- User-programmable alarm thresholds
- Graphic LCD shows real-time readings, graph and current status
- Resettable Min/Max readings may be viewed on the LCD
- User set audible alarm
- Highly visible confidence/alarm LEDs
- Supplied with user replaceable ½ AA batteries



The EL-GFX-1 standalone USB data logger measures and stores up to 252,928 temperature readings over a -30 to +80°C (22 to +176°F) range and at a resolution of 0.1°C. Using the Windows control software (available as a free-download from [www.easylogusb.com](http://www.easylogusb.com)), users can quickly set up the data logger and view downloaded data by connecting the device to the PC's USB port using the supplied cable.

The data logger features a high-contrast graphic LCD and three-input buttons. This allows users to start, stop and restart the data logger using on-screen menus. This menu also provides real-time analysis of data either as a data summary (showing highest & lowest readings and alarm conditions) or as a graph that updates as new data is added. The Max and Min readings and also the Time and Date these are valid from, can be displayed on the LCD (  info button). If desired, the user can then reset the Max/Min shown on this screen of the LCD. Each time these maxima and minima are reset whilst logging, an "Event Marker" is created in the data. When the data has been downloaded to a PC these Events can be viewed on the graph (Mark Events), they also appear in the data file - associated with the corresponding log when the reset took place. For certain applications where procedures mandate that a regular physical check of the logger / stats have taken place - this can be useful as an audit / validation tool. Multiple data logging sessions can be stored on the device ready for upload to a PC at a later date.

The data logger's robust design provides IP-67 waterproof protection and the two replaceable ½AA batteries typically allow logging for up to one year.

Specifications	Minimum	Typical	Maximum	Unit
Measurement range	-30 (-22)		+80 (+176)	°C (°F)
Internal resolution		0.1 (0.1)		°C (°F)
Accuracy (overall error)		±0.1 (±0.2)*	±0.75 (±1.5)	°C (°F)
Logging rate	every 10s		every 1hr	-
Operating temperature range**	-30 (-22)		+80 (+176)	°C (°F)
2 x ½AA 3.6V Lithium Battery Life		1***		Year

\* At 25 °C. See Temperature Accuracy curve on page 4

\*\* At temperatures below -5 °C the LCD will exhibit slower response times. The LCD will be disabled at temperatures under -20 °C and above 70 °C

\*\*\* At 25 °C and 10 minute logging rate with no alarm LEDs or sounder and minimal LCD use

# EL-GFX-1


## Temperature Data Logger with Graphic LCD Screen

### EL-WIN-USB (CONTROL SOFTWARE)

Lascar's Easylog USB control software is available to download from [www.easylogusb.com](http://www.easylogusb.com). Easy to install and use, the control software runs under Windows XP, Vista and Windows 7. The software is used to set-up the data logger as well as download, graph and export data to Excel. Each stored logging session is saved as a separate file.

The software allows the following parameters to be configured:

- Logger name
- Measurement parameter (°C or °F)
- Logging Rate (user-selectable between 10 seconds and 1 hour)
- High and low temperature alarms
- Immediate, delayed, push-button or temperature triggered start mode
- Disable or enable LEDs and sounder with delayed activation
- Display and backlight behaviour after button press

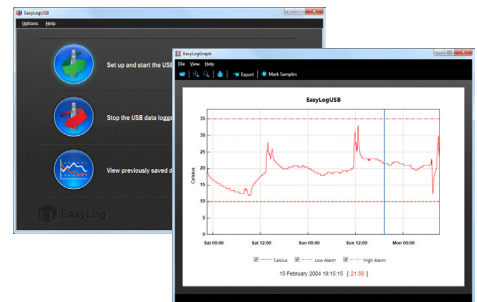

The latest version of the control software may be downloaded free of charge from [www.easylogusb.com](http://www.easylogusb.com)

### DIMENSIONS











All dimensions in mm (inches)



# EL-GFX-1

## Temperature Data Logger with Graphic LCD Screen

### MENU BUTTON FUNCTIONS AND LED SCREEN INDICATION

 Button	 Time	 Value	<b>START</b> <ul style="list-style-type: none"><li>Loggers can be started immediately on a button press, delayed to a specific time or delayed to specific temperature reading</li></ul>	 • Audible alarm can be muted if required	<b>MUTE ALARM</b>	
			 • The logger can be stopped using the buttons	  • Summary screen displays max/min log and last log. Reset function clears summary if required	<b>STOP</b>	<b>SUMMARY DATA</b>
  • Data can be displayed on screen in tabular or graphical format			<b>DISPLAY DATA</b>	 • "Locked" mode can be unticked during PC set-up if required • When in locked mode, the logger can only be stopped and re-started using a PC loaded with the unit's configuration software	<b>LOCK MENU BUTTONS</b>	

### BATTERY REPLACEMENT

We recommend that you replace the batteries every 12 months, or prior to logging critical data.

The EL-GFX-1 does not lose its stored readings when the batteries are discharged or when the batteries are replaced; however, the data logging process will be stopped. If the batteries are changed within a 2 minute window the EL-GFX-1 will retain its settings (internal clock and logging mode). This will allow logging to be restarted without additional connection to a PC via USB.

Only use 2 x 3.6V ½AA lithium batteries. Do not mix battery types and do not mix new and old batteries. Before replacing the batteries, unplug the EL-GFX-1 from the PC.


### WARNING

Handle lithium batteries carefully, observe warnings on battery casing. Dispose of in accordance with local regulations.

# EL-GFX-1

## Temperature Data Logger with Graphic LCD Screen

### TEMPERATURE ACCURACY

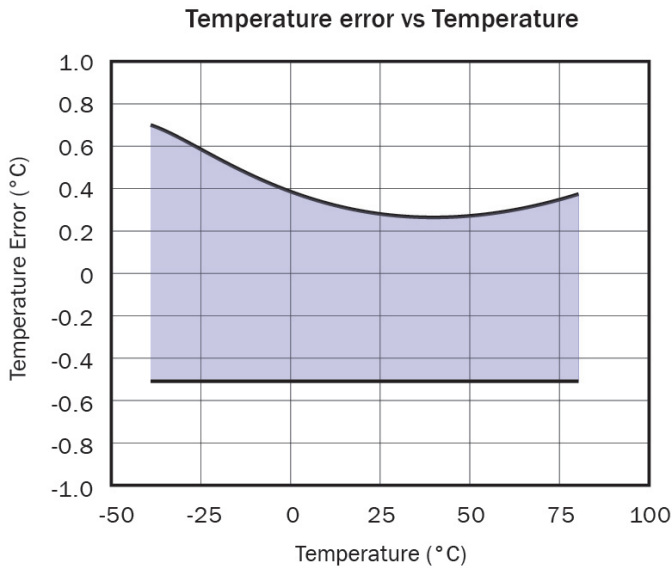

Module House  
Whiteparish, Salisbury  
Wiltshire SP5 2SJ  
UK  
T +44 (1794) 884567  
F +44 (1794) 884616  
E sales@lascar.co.uk

4258 West 12th Street  
Erie  
PA 16505  
USA  
T +1 (814) 835 0621  
F +1 (814) 838 8141  
E us-sales@lascarelectronics.com

8th Floor, China Aerospace Centre  
143 Hoi Bun Road  
Kwun Tong, Kowloon  
HONG KONG  
T +852 2797 3219  
F +852 2343 6187  
E saleshk@lascar.com.hk



[www.lascarelectronics.com](http://www.lascarelectronics.com)



## X-ON Electronics

Largest Supplier of Electrical and Electronic Components

*Click to view similar products for [Environmental Test Equipment](#) category:*

*Click to view products by [Lascar](#) manufacturer:*

Other Similar products are found below :

[CW40](#) [F150C10E3DRT](#) [F150LTC20](#) [F150CD10E2](#) [F150L75](#) [F150LRS](#) [S-11](#) [FLUKE-LDG](#) [382153](#) [FM100](#) [RH210](#) [382253](#) [MO290-P](#)  
[GEO-CABLE-REEL-50M](#) [T197914](#) [RD300-L](#) [IR11BD](#) [IR11GM](#) [IR12GM](#) [IR21BD](#) [IR31CE](#) [IR32BC](#) [IR33BC](#) [MP7217TC](#) [NGM-1](#) [SGX-](#)  
[7NH3](#) [UT381](#) [F150-SLC50](#) [AW-CO-1000](#) [AW-NmHc-100](#) [3.000.401](#) [AX-7535](#) [CS-9S6SS-A](#) [P 2800 A](#) [P 2801](#) [P 2802](#) [P 5039](#) [P 5130](#) [P](#)  
[5055](#) [P 5060](#) [P 5065](#) [P 5086](#) [P 5090](#) [P 5110](#) [P 5115](#) [P 5135](#) [P 5140](#) [P 5145](#) [P 5150](#) [P 5160](#)