

# METRISO XTRA

## High-Precision

## Insulation, Low Resistance and Voltage Measurement Instrument

3-349-816-03  
2/7.19

- Insulation measurement per IEC/EN 61557-2
- Test voltages in fixed increments, variable or as a ramp  
50 V, 100 V, 250 V, 500 V, 1000 V
- Polarization index and absorption ratio
- **Intelligent filter** – measurement-dependent and precise activation for the measurement of very high resistances
- Backlit dot matrix display for measured and limit values
- Signalling of dangerous contact voltage
- **Acoustic** signalling when limit value is exceeded
- **Detection of interference voltage** in switch position OFF
- **Overvoltage protection**  
Protects the instrument in the event of inadvertent connection to mains power  
– Fuse link for all resistance measuring ranges  
– Electronic fuse for the protection of low resistance and resistance measurement  $R_{LO}$  and R
- Low resistance measurement per IEC 61557-4
- Guard terminal for compensating surface current
- **Compact and rugged** For service calls under harsh conditions
- **One measuring point self-test with test resistance of 10 M $\Omega$**  per IEC/HD 60364-6 / EN 50110
- Bidirectional interface to ETC (report generating software)



**CAT IV CE**



### Application

The insulation and resistance measuring instrument allows for quick and effective testing of protective measures in accordance with DIN VDE 0100, ÖVE-EN 1 (Austria), NIV/NIN SEV 1000 (Switzerland) and regulations specific to other countries as well. The instrument complies with IEC/EN 61557 regulations:

Part 1: General requirements

Part 2: Insulation resistance

Part 4: Resistance at earthing conductors, protective conductors and equipotential bonding

Part 10: Electric safety in low voltage systems up to AC 1000 V and DC 1500 V – Equipment for testing, measuring and monitoring protective measures

as well as requirements per VDE 0701-0702:

Repair, modification and testing of electrical devices

#### The insulation measuring instruments are suitable for the following tasks:

- Measurement of insulation resistance at voltage-free devices and systems, up to 1000 V depending upon variant
- Checking of test objects for absence of voltage in systems up to 1 kV
- Testing of the resistance of earthing conductors, protective conductors and equipotential bonding
- Testing of electrostatic discharge capacity at floor coverings (using shielded measurement cables) – EN 1081
- With the so-called 1 mA test per DIN VDE 0845/EN 61645, the instrument also allows to perform on-site tests of the response voltage of overvoltage components (varistors, Zener diodes, etc.) of requirement categories B and C / SPD Type 2 and 3) and to evaluate the test results in accordance with manufacturer's data.

### Features Overview

METRISO XTRA	Article number	M550S
<b>Measurements</b>		
$R_{ISO}$ Ufixed = 50, 100, 250, 500, 1000 V (Limit values VDE 0100)		✓
$R_{ISO}$ Uvariable = 50 ... 1000 V (Limit value+ = 1 MOhm)		✓
$R_{ISO}$ Uramp = 50 ... 1000 V Display of breakdown voltage		✓
PI/DAR Polarization Index Measurement		✓
R 10 ... 10 k $\Omega$		✓
$R_{LO}$ 0,01 ... 10 $\Omega$ (Limit value VDE 0100)		✓
U 0 ... 1000 V		✓
<b>Display functions</b>		
Backlit display		✓
<b>Limit value LED (green/red) for:</b> Additional acoustic signal, limit values per VDE 0100		$R_{ISO}$ $R_{LO}$
<b>Limit value LED Uramp for:</b> Signalling of ramp sequence		$R_{ISO}$
<b>LED for dangerous contact voltage</b> (when switched off)		✓
Battery level display		✓
<b>Special functions</b>		
Discharge of capacitive devices under test		✓
Safety shutdown (UBatt < 8 V)		✓
Data storage in the instrument (database max. 50,000 structural elements)		✓
<b>Features</b>		
Measuring category CAT II 1000 V / CAT III 600 V / CAT IV 300 V		✓
10 M $\Omega$ test resistor		✓
Terminals: charging socket, USB interfacee (slave), RS232 interface		✓
DAKKS calibration certificate		✓

# METRISO XTRA

## High-Precision

## Insulation, Low Resistance and Voltage Measurement Instrument

### Polarization Index

A polarization index test is recommended for electrical machines with coil modules (generator and motor coils). This procedure involves expanded testing of insulation resistance. A reduced insulation resistance is an indication of humidity absorption and fouling.

To this end, the DC measuring voltage of the METRISO XTRA is applied to the insulation for a duration of 10 minutes. The respective measured value is read after one and after ten minutes. If the insulation is faultless, the value measured after ten minutes is higher than the value measured after one minute. The relationship between the two measurement values is the polarization index.

Charged material within the insulation is aligned due to the application of DC measuring voltage over a long period of time, resulting in polarization. The polarization index indicates whether or not the charged material contained in the insulation can still be moved, thus allowing for polarization. This, in turn, is an indication of the condition of the insulation. The more the charged material can be moved, the better is the state of the insulation.

### Discharging of Capacitive DUTs

Capacitive devices under test such as cables and coils which may charge up to test voltage are discharged via the test instrument while the voltage decrease can be monitored at the display.

### Data Management and Report Generation

A complete distribution structure with customer, building and distributor data can be set up in the test instrument. This structure allows for the assignment of measurements to the distributors of different buildings and customers.

### Intelligent filter

Measurement-dependent and precise activation for the measurement of very high resistances with:

- beating, i. e. compensation of  $16^{2/3}$  Hz and 50 Hz interferences
- attenuation of capacitive influences from power cables, etc.
- suppression of electric field influences

## Characteristic Values

### METRISO XTRA

Meas. Qty.	$U_{ISO}$	Range	Measuring Range	Resolution	Open-Circuit Voltage $U_{0max}$	Test Current	Intrinsic Uncertainty	Measuring Uncertainty	Overload Capacity
$R_{ISO}$	50 V 100 V 250 V / 500 V 1000 V	100 k	10 k $\Omega$ ... 99.9 k $\Omega$	0.1 k	50 V / 100 V: 1.25 $U_{ISO}$  250 V / 500 V / 1000 V: 1.1 $U_{ISO}$	$I_N = 1$ mA  $I_K \leq 5$ mA	$\pm(5\% \text{ rdg.} + 3 \text{ d})$	$\pm(7\% \text{ rdg.} + 3 \text{ d})$	1000 V AC/DC TRMS
		1 M	100 k $\Omega$ ... 999 k $\Omega$	1 k					
		10 M	1.00 M $\Omega$ ... 9.99 M $\Omega$	10 k					
		100 M	10.0 M $\Omega$ ... 99.9 M $\Omega$	100 k					
		1 G	100 M $\Omega$ ... 999 M $\Omega$	1 M					
		10 G	1.00 G $\Omega$ ... 9.99 G $\Omega$	10 M					
		100 G	10.0 G $\Omega$ ... 99.9 G $\Omega$	100 M					
		1 T	100 G $\Omega$ ... 999 G $\Omega$	1 G			$\pm(8\% \text{ rdg.} + 3 \text{ d})^1$ $\pm(25\% \text{ rdg.} + 5 \text{ d})^1$	$\pm(10\% \text{ rdg.} + 3 \text{ d})^1$ $\pm(50\% \text{ rdg.} + 20 \text{ d})^1)^2$	
$U_{AC/DC}$		100 V	10.0 V ... 99.9 V	0.1 V	—	—	$\pm(2.5\% \text{ rdg.} + 3 \text{ d})$	$\pm(5\% \text{ rdg.} + 3 \text{ d})$	1000 V AC/DC TRMS <sup>3)</sup>
		1000 V	100 V ... 999 V	1 V					
$R_{LO}$		10 $\Omega$	0.17 ... 9.99 $\Omega$	0.01 $\Omega$	4 V < $U_0$ < 6 V	200 mA $\leq I$ $I \leq 260$ mA <sup>4)</sup>	$\pm(2.5\% \text{ rdg.} + 3 \text{ d})$	$\pm(5\% \text{ rdg.} + 3 \text{ d})$	1000 V AC/DC TRMS
$R$	Display range as of 01.0 $\Omega$	100 $\Omega$	10.0 ... 99.9 $\Omega$	0.1 $\Omega$	$U_0 \text{ max. } 15 \text{ V}$	1 mA $\leq I$ $I \leq 1.3$ mA	$\pm(2.5\% \text{ rdg.} + 3 \text{ d})$	$\pm(5\% \text{ rdg.} + 3 \text{ d})$	1000 V AC/DC TRMS
		1 k $\Omega$	100 ... 999 $\Omega$	1 $\Omega$					
		10 k $\Omega$	1.00 ... 9.99 k $\Omega$	10 $\Omega$					

<sup>1)</sup> the indicated accuracy is only achieved with the shielded high-resistance measuring cable KS-C (article no. Z541F)\* as optional accessory.

<sup>4)</sup> up to 5  $\Omega$

<sup>2)</sup> does not conform to DIN EN 61557-2

<sup>3)</sup> display range up to 1.2 kV

### Breakdown Voltage (Uramp)

Parameter	Range	Intrinsic Uncertainty	Measuring Uncertainty
Voltage range	100 ... 1000 V	$\pm(10\% \text{ rdg.} + 8 \text{ d})$	$\pm(15\% \text{ rdg.} + 10 \text{ d})$
Rise time	5 ... 30 s	—	—
Measuring duration	1 ... 120 s / auto / permanent measurement	—	—

### Polarization Index (PI), Absorption Ratio (DAR)

	t1	t2	Limit
PI	01:00 min	10:00 min	> 4.0 min / > 3.0 min / > 2.0 min / > 1.5 min / > 1.1 min / > 1.0 min
DAR	00:30 min	01:00 min	> 1.60 min / > 1.25 min

PI and DAR are calculated values. The specifications of the insulation measurement apply.

### Reference Conditions

Reference temperature	+ 23 °C $\pm$ 3 K
Relative humidity	40 ... 75%
Measured quantity frequency	45 Hz ... 65 Hz
Measured quantity waveshape	Sine, deviation between TRMS and rectified value < 1%
Battery voltage	9.5 V $\pm$ 0.1 V
Test resistor	10 M $\Omega$ $\pm$ 1%

### Electrical Safety

Protection class	II per IEC/EN 61 010-1
Pollution degree	2
Measuring category	CAT II 1000 V / CAT III 600 V / CAT IV 300 V
Fuses	
Fuse link	FF315mA/1000V, effective in all resistance measuring ranges, 1 additional replacement fuse in the battery compartment
Elektronic fuse	for protecting low-resistance and resistance measurement $R_{LO}$ and R


### Ambient Conditions

Accuracy temperature range	0 ... +40 °C
Operating temperatures	-10 ... +50 °C
Storage temperatures	-25 ... +70 °C (without batteries)
Relative humidity	up to 75% (max. 85% during storage/transport), no condensation allowed
Elevation	max. 2000 m
Calibration interval	1 year (recommended)

### Electromagnetic Compatibility (EMC)

Interference emission	EN 61326-1:2013 class B
Interference immunity	EN 61326-1:2013

### Displays

Digital display	Multiple display via dot matrix 128 x 128 pixels, backlit (transflective); Dimensions: 65 mm x 65 mm
LED Limit	LED lights up red to indicate an exceeded limit value LED lights up green to indicate adherence to the limit value
LED 	LED lights up red to indicate the presence of an external voltage (with the instrument switched off) or high test voltage during insulation measurement (Riso/Rins, PI and DAR) at the measuring terminals
LED Uramp	LED lights up green to indicate the ramp sequence, LED lights up red to indicate the interruption of the ramp sequence (e. g. in case of breakdown)


### Mechanical Design

Dimensions	225 mm x 130 mm x 140 mm
Weight	approx. 1.5 kg with (rechargeable) batteries
Protection	Housing IP 52, measurement cables and connectors IP 40 per DIN VDE 0470 part 1/ EN 60529

#### Extract from table on the meaning of IP codes

IP XY (1 <sup>st</sup> digit X)	Protection Against Foreign Object Entry	IP XY (2 <sup>nd</sup> digit Y)	Protection Against Penetration by Water
2	≥ 12.5 mm dia.	2	Dripping (at 15° angle)
3	≥ 2.5 mm dia.	3	Spraying water
4	≥ 1.0 mm dia.	4	Splashing water
5	Dust protected	5	Jet-water

### Power Supply

Batteries (rechargeable batteries as an option)	8 ea. 1.5 V mignon cell (8 ea. size AA) (alkaline manganese per IEC LR14) Rechargeable batteries: we recommend only using the pack of rechargeable batteries article no. Z502H
Battery charger Z502R (as an option)	Broad band charger with jack plug, Input: 100 ... 240 V AC; Output: 16.5 V DC, 1 A (Mascot)
Nominal range of use	8.5 ... 12 V
Battery test	Battery capacity display with battery symbol in 4 segments „  “. Querying of momentary battery voltage via menu function.
Battery saver circuit	Automatic shutdown of display illumination after 10 ... 30 seconds (after the last time the rotary switch is actuated) can be set in the SETUP menu. The test instrument is automatically switched to the <b>standby mode</b> when the measured value remains unchanged for approx. 15 minutes and none of the controls are activated during this time. The instrument switches off <b>automatically</b> if the measured value remains constant for a lengthy period of time and no key or rotary switch is activated for seconds during on-time.
Service life	for $R_{INS}$ (1000 V/1 M $\Omega$ ), $R_{LO}$ with 25 s on-time and 1 subsequent measurement each for a duration of 5 seconds: – with a set of batteries (alkaline manganese): 400 measurements – with a set of rechargeable batteries (2200 mAh): 650 measurements
Safety shutdown	If supply voltage is too low ( $U < 8$ V), the instrument is switched off, or cannot be switched on.
Charging socket	Inserted rechargeable batteries can be directly recharged by connecting a charger to the charging socket: Charger Z502R
Charging time	approx. 2 hours *

\* maximum charging time for totally depleted batteries.  
A timer in the charger restricts the charging time to a maximum of 4 hours

# METRISO XTRA

## High-Precision

## Insulation, Low Resistance and Voltage Measurement Instrument

### Data Interfaces

Type	USB slave for PC connection
Type	RS232 for barcode and RFID scanners

### Applicable Regulations and Standards

<b>IEC 61010-1/ EN 61010-1 VDE 0411-1</b>	Safety requirements for electrical equipment for measurement, control and laboratory use Part 1: General requirements (IEC 61010-1:2010 + Cor.:2011); German edition EN 61010-1:2010 Part 31: Safety requirements for handheld measuring and testing accessories (IEC 61010-031:2002 + A1:2008); German edition EN 61010-031:2002 + A1:2008
<b>IEC 61557/ EN 61557/ VDE 0413</b>	Part 1: General requirements (IEC 61557-1:2007); German edition EN 61557-1:2007 Part 2: Insulation resistance (IEC 61557-2:2007); German edition EN 61557-2:2007 Part 4: Resistance of earth conductors, protective conductors and equipotential bonding conductors (IEC 61557-4:2007); German edition EN 61557-4:2007 Part 10: Electrical safety in low voltage systems up to AC 1000 V and DC 1500 V – Equipment for testing, measuring or monitoring protective measures (IEC 61557-10:2000); German edition EN 61557-10:2001
<b>EN 1081</b>	Testing of electrostatic discharge capacity for floor coverings in potentially explosive atmospheres
<b>EN 60529 VDE 0470-1</b>	Test instruments and test procedures Degrees of protection provided by enclosures (IP code)
<b>DIN EN 61326-1 VDE 0843-20-1</b>	Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 1: General requirements

### Scope of delivery

- 1 Insulation and resistance measuring instrument
- 1 DAkkS calibration certificate
- 1 Set of batteries
- 1 Carrying strap
- 1 Alligator clip
- 1 Cable set KS17-4
- 1 USB cable
- 1 Condensed operating instructions
- 1 Supplement Safety Information
- Detailed operating instructions for download from our website at [www.gossenmetrawatt.com](http://www.gossenmetrawatt.com)

### Accessories (not included)

#### Akku-Pack Master Z502H



#### Charger Z502R



#### ISO Kalibrator 1

Calibration adapter for the rapid, efficient testing of the accuracy of measuring instruments for insulation resistance and low-impedance resistances.



#### Cable Set KS-C

Cable set consisting of measurement cable and high resistance measuring cable, for measurements in the G-Ω range.



#### Cable Set KS24

Cable set KS 24 consists of a 4 m long extension cable with a permanently mounted test probe at one end and a contact protected socket at the opposite end, as well as an alligator clip for plugging onto the test probe.

#### TELEARM 120 Telescoping Rod



#### Case TELEARM







### Floor Probe

The 1081 floor probe can be used for measuring the resistance of insulating floors in accordance with DIN VDE 0100 Part 600 and EN 1081.

### TR25II Cable reel (Z503X)



25 m measurement cable coiled onto a plastic drum. Connection to the inside end of the cable is made possible with two sockets integrated into the drum. The other end is equipped with a banana plug.

### TR50II Cable reel (Z503Y)



50 m measurement cable coiled onto a plastic drum. Connection to the inside end of the cable is made possible with two sockets integrated into the drum. The other end is equipped with a banana plug.

### Operating Case METRISO G (Z550C)




### Test Probe for Remote Triggering Z550A

Connection example: module slot for INTRO / BASE / TECH / PRO / XTRA



### Magnetic measuring contacts (patent) with magnetic strain relief (Z502U)

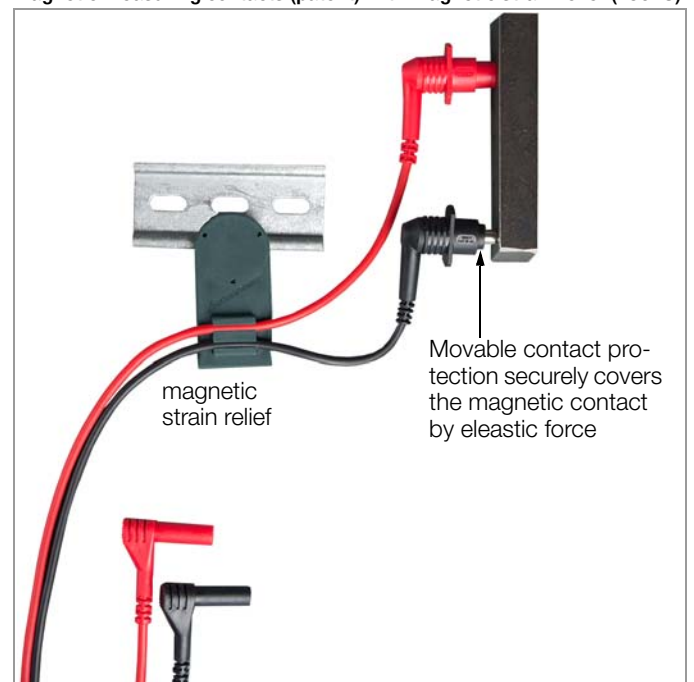

# METRISO XTRA

## High-Precision

## Insulation, Low Resistance and Voltage Measurement Instrument

### Order Information

Description	Type	Article Number
Insulation measuring instrument for DIN VDE 0100, ÖVE-EN 1 (Austria), NIV/NIN SEV 1000 (Switzerland), complies with IEC/EN 61 557/VDE 0413, parts 1+2+4+10		
Test voltage up to 1000 V, voltage measurement up to 1000 V, low-resistance measurement, measurement of polarity and absorption index	METRISO XTRA	M550S
METRISO XTRA inclusive Test Probe for Remote Triggering (Z550A) and Operating Case (Z550C)	METRISO XTRA-Set	M551S
<b>Accessories (not included)</b>		
8 LSD NiMH rechargeable batteries with reduced self-discharging (AA), 2000 mAh with sealed cells	Akku-Pack Master	Z502H
Charger for charging the rechargeable batteries inserted in the METRISO XTRA Broad band charger Input: 100 ... 240 V AC; Output: 16.5 V DC, 1 A	Z502R	Z502R
Calibration adapter for testing the accuracy of instruments used for measuring insulation resistances and low-resistance for test voltages up to 1000 V (per VDE 0413, part 1, 2 and part 4)	ISO-Kalibrator 1	M662A
Cable set consisting of measurement cable and shielded high resistance measurement cable, for measurements in the GΩ range	KS-C	Z541F
Triangular probe for floor measurements per EN 1081, DIN VDE 0100	1081 probe	GTZ3196000R0001
Cable set consisting of a 4 m long extension cable with a permanently attached test probe at one end and a contact protected socket at the other end, and 2 alligator clips which can be plugged onto the test probe	KS24	GTZ3201000R0001
Telescoping rod for RLO and RISO measurement, CAT III 600 V / CAT IV 300 V, 1 A, retracted/extended 53,3 cm/120 cm, 190 g	TELEARM 120	Z505C
Telescoping rod for RLO and RISO measurement, CAT III 600 V / CAT IV 300 V, 1 A, retracted/extended 73,5 cm/180 cm, 250 g	TELEARM 180	Z505D
Case TELEARM for Telearm 120/180, 920 x 170 mm	Case TELEARM	Z505E
Cable reel for low-resistance and earth-resistance measurement, 25 m	TR25II	Z503X
Cable reel for low-resistance and earth-resistance measurement, 50 m	TR50II	Z503Y

Description	Type	Article Number
Test probe with START/STOP key and an additional key for illuminating the measuring point, including shielded cable and test probe holder for carrying belt	Test Probe for Remote Triggering METRISO G	Z550A
Ever-ready case for METRISO INTRO / BASE / TECH / PRO / XTRA with external pocket for measurement cable	Operating Case METRISO G	Z550C
Magnetic Measuring contacts with contact protection – Set with magnetic holder, measurement contacts 5,5 mm in diameter insulated, CAT III 1.000 V / 4 A, temperature between -10 °C and 60 °C, under standard conditions and flat-head screws holding force 1.200 g vertical to contact area; measuring instrument connector: angled multilam plug according (for METRISO G series)	Set 1 – Magnetic Measuring Tips	Z502U
<b>Description</b>		
<b>Type</b>		
<b>Article Number</b>		
<b>Report Generation Accessories (not included)</b>		
Barcode scanner for RS232 interface (laser sensor), variable barcode length, increased scanning accuracy, with coiled cable	Barcode-Profiscanner-RS232	Z502F
RFID read/write for RS232 interface (13.56 MHz)	SCANBASE RFID	Z751G
For further information on barcode scanner, barcode printer and RFID scanner see separate datasheet „ID systems“		
<b>PC Analysis Software</b>		
Additional information regarding software is available on the Internet at <a href="http://www.gossenmetrawatt.com">http://www.gossenmetrawatt.com</a> (→ Software → Product specific Software → Software for Testers)		

For additional information on accessories, please refer to

- our website [www.gossenmetrawatt.com](http://www.gossenmetrawatt.com)

Edited in Germany • Subject to change without notice • A pdf version is available on the Internet

 **GOSSEN METRAWATT**

GMC-I Messtechnik GmbH  
Südwestpark 15  
90449 Nürnberg • Germany

Phone +49 911 8602-111  
Fax +49 911 8602-777  
E-Mail [info@gossenmetrawatt.com](mailto:info@gossenmetrawatt.com)  
[www.gossenmetrawatt.com](http://www.gossenmetrawatt.com)

## **X-ON Electronics**

Largest Supplier of Electrical and Electronic Components

*Click to view similar products for [Gossen Metrawatt](#) manufacturer:*

Other Similar products are found below :

[1717V1260](#) [1720V0050](#) [DUSPOL ANALOG 1000](#) [DUSPOL DIGITAL 1000](#) [DUSPOL EXPERT 1000](#) [METRACLIP 41](#) [METRACLIP 41/410 CASE](#) [METRAHIT AM BASE](#) [METRAHIT AM PRO](#) [METRAHIT AM XTRA](#) [METRAHIT WORLD](#) [METRALINE DM41](#) [METRALINE DM61](#) [METRALINE DM62](#) [METRAMAX2](#) [METRAPHASE 1](#) [METRAVOLT 12D +L](#) [METRISO PRO](#) [PROFISAFE 690L](#) [U270B](#) [U528D](#)