

Keysight 16089A/B/C Kelvin Clip Leads

Operation and
Service Manual

Notices

© Keysight Technologies
1991–2020

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies, Inc. as governed by United States and international copyright laws.

Trademark Acknowledgments

Manual Part Number

16089–90030

Edition

Edition 7, January 2020

Printed in Malaysia

Published by:

Keysight Technologies International
Japan G.K,
1–3–3 Higashikawasaki-cho
Chuo-ku
Kobe-shi, Hyogo, Japan

Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED “AS IS,” AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS

COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Declaration of Conformity

Declarations of Conformity for this product and for other Keysight products may be downloaded from the Web. Go to <http://www.keysight.com/go/conformity>. You can then search by product number to find the latest Declaration of Conformity.

U.S. Government Rights

The Software is “commercial computer software,” as defined by Federal Acquisition Regulation (“FAR”) 2.101. Pursuant to FAR 12.212 and 27.405–3 and Department of Defense FAR Supplement (“DFARS”) 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public. Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at

<http://www.keysight.com/find/sweula> The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight: (1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release,

perform, display, or disclose commercial computer software or commercial computer software documentation. No additional government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no greater than Limited Rights as defined in FAR 27.401 or DFARS 227.7103–5 (c), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Table of Contents

1. General Information	
Introduction	5
Using the 16089A/B/C	5
Product Description	6
Accessories Supplied	6
Operating and Safety Precautions	7
Operating	7
Service	7
Specifications	8
Supplemental Performance Characteristics	9
Supplemental Performance Characteristics of 16089A	9
Supplemental Performance Characteristics of 16089B	9
Supplemental Performance Characteristics of 16089C	9
2. Preparation for Use	
Introduction	11
Initial Inspection	11
16089A	12
16089B	13
16089C	14
Ambient Environmental Considerations	15
Operating and Storage	15
Connecting the Test Leads for Use	15
Packaging the Test Leads	15
3. Operation	
Introduction	17
Test Leads Features	17
16089A/B/C	17
OPEN and SHORT Compensation	18
Operation	19
4. Service	
Introduction	21
Replaceable Parts	22
16089A Replaceable Parts	22
16089B Replaceable Parts	23
16089C Replaceable Parts	24

Contents

1 General Information

Introduction

The purpose of this manual is to enable you to use your Keysight 16089A/B/C Kelvin Clip Leads efficiently and confidently. This manual contains both general and specific information. To use the 16089A/B/C to perform a specific function (without having to read the entire manual), follow the directions in **“Using the 16089A/B/C”**.

Using the 16089A/B/C

The 16089A/B/C has been designed to operate specifically with the LCR Meter.

- To install the 16089A/B/C, turn to **Chapter 2**.
- To operate the 16089A/B/C, turn to **Chapter 3**.
- To order replaceable parts for the 16089A/B/C, turn to **“Replaceable Parts”** in **Chapter 4**.

Product Description

The 16089A/B/C has been designed to operate specifically with the following four-terminal-pair type LCR meters and impedance analyzers.

The 16089A/B/C make it possible to measure odd-shaped components that cannot be measured with conventional test fixtures. The 16089A, 16089B, and 16089C consist of a direct attachment, four-terminal-pair type test leads that are equipped with two insulated Kelvin clips. Three sizes of Kelvin clips are provided. The 16089A Kelvin Clip Leads is equipped with two large Kelvin clips, the 16089B Kelvin Clip Leads is equipped with middle size clips and the 16089C Kelvin Clip Leads is equipped with small size clips.

Accessories Supplied

The following accessories are supplied with the 16089A/B/C:

Table 1-1

Furnished Accessories

Description	Part Number	Quantity
Operation and Service Manual (this manual) ¹	Option ABA	1

1. The manual is furnished only Option ABA is ordered.

Operating and Safety Precautions

Operating

You need to observe only normal precautions in handling and operating the 16089A/B/C. Do not exceed the operating input power, voltage and current level and signal type appropriate for the instrument being used, refer to your instrument's operation manual.

CAUTION

Electrostatic discharge (ESD) can damage the highly sensitive microcircuits in your instrument. ESD damage is most likely to occur as the test leads are being connected or disconnected. Protect them from ESD damage by wearing a grounding strap that provides a high resistance path to ground. Alternatively, ground yourself to discharge any static charge built-up by touching the outer shell of any grounded instrument chassis before touching the test port connectors.

Never touch the test clip contacts.

Use a work station equipped with an anti-static work surface.

Service

The voltage levels found in these test leads when used with the intended instruments do not warrant more than normal safety precautions for operator safety. Nevertheless, service should be performed only by qualified personnel.

Specifications

This section lists the complete 16089A/B/C specifications. These specifications are the performance standards and limits against which the 16089A/B/C is tested. When shipped from the factory, the 16089A/B/C meets the following specifications:

Maximum dc Bias Voltage	$\pm 42\text{V}$ peak max
Frequency Range	5Hz to 100kHz
Operating Temperature	0 to 55°C
Operating Humidity	$\leq 95\%$ RH (@40°C)
Non-operating Temperature	-40 to 70°C
Non-operating Humidity	$\leq 95\%$ RH (@40°C)
Weight	300g
Cable length	0.94m

Supplemental Performance Characteristics

This section gives supplemental performance characteristics. Supplemental performance characteristics are not specifications, but are typical characteristics included as additional information for the operator. Supplemental performance characteristics are not guaranteed.

Supplemental Performance Characteristics of 16089A

Applicable DUT size

Diameter of DUT's terminals $\leq 15\text{mm}$

Supplemental Performance Characteristics of 16089B

Applicable DUT size

Diameter of DUT's terminals $\leq 7.9\text{mm}$

Length of DUT's terminals $\geq 3\text{mm}$

Supplemental Performance Characteristics of 16089C

Applicable DUT size

Diameter of DUT's terminals $\leq 1\text{mm}$

Space between DUT's terminals $\geq 2\text{mm}$

Length of DUT's terminals $\geq 2\text{mm}$

General Information
Supplemental Performance Characteristics

2 Preparation for Use

Introduction

This chapter explains how to install the Keysight 16089A/B/C Kelvin Clip Leads. The topics covered include initial inspection, ambient environmental considerations, connecting the test leads for use, and repackaging the test leads for shipment.

Initial Inspection

These test leads have been carefully inspected electrically and mechanically before being shipped from the factory. They should be in perfect physical condition, no scratches, dents or the like. They should also be in perfect electrical condition. Verify this by carefully performing an incoming inspection to check the test lead set for signs of physical damage and missing contents. If any discrepancy is found, notify the carrier and Keysight Technologies. Your Keysight Technologies sales office will arrange for repair and replacement without waiting for the claim to be settled.

- Inspect the shipping container for damage. Keep the shipping materials until the inspection is completed.
- Verify that the shipping container contains everything shown in **Figure 2-1**, **Figure 2-2**, **Figure 2-3**, and **Figure 2-4** and listed in **Table 2-1**, and **Table 2-2**, **Table 2-3**.
- Inspect the exterior of the 16089A/B/C for any signs of damage.

16089A

Figure 2-1 16089A Product Overview



Table 2-1 Contents of 16089A

Description	Keysight Part Number	Qty
Kelvin Clip Leads 1m	Option 800 ¹	1
Kelvin Clip Leads 2m	Option C20 ¹	
Operation and Service Manual (this manual) ²	Option ABA	1

1. Either option 800 or C20 will be furnished.
2. Operation and Service Manual is not shown in **Figure 2-1** and furnished only Option ABA is ordered.

16089B

Figure 2-2 16089B Product Overview



Table 2-2 Contents of 16089B

Description	Keysight Part Number	Qty
Kelvin Clip Leads 1m	Option 800 ¹	1
Kelvin Clip Leads 2m	Option C20 ¹	
Operation and Service Manual (this manual) ²	Option ABA	1

1. Either option 800 or C20 will be furnished.
2. Operation and Service Manual is not shown in **Figure 2-2** and furnished only Option ABA is ordered.

16089C

Figure 2-3 16089C Product Overview



Table 2-3 Contents of 16089C

Description	Keysight Part Number	Qty
Kelvin IC Clip Leads	16089-60603 ¹	1
Operation and Service Manual (this manual) ²	Option ABA	1

1. Keysight internal-only part number.
2. Operation and Service Manual is not shown in **Figure 2-3** and furnished only Option ABA is ordered.

Ambient Environmental Considerations


Operating and Storage

The 16089A/B/C must be operated within an ambient temperature range of 0°C to 55°C and relative humidity up to 95% at 40°C (non-condensing).

The 16089A/B/C may be stored within a temperature range of -40°C to +70°C, and at a relative humidity of up to 95% at +40°C (non-condensing).

Connecting the Test Leads for Use

Figure 2-4 Connecting the Test Leads

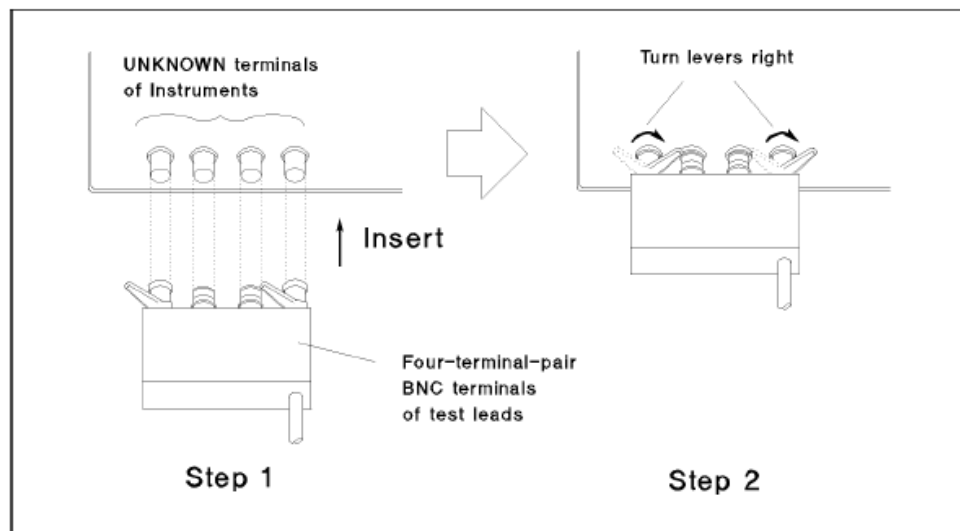

Packaging the Test Leads

If shipment to a Keysight Technologies service center is required, each test lead set should be repackaged using the original factory packaging materials.

Alternatively, comparable packaging materials may be used. Wrap the test leads in heavy paper and pack in anti-static plastic packaging material. Use sufficient shock absorbing material on all sides of the 16089A/B/C to provide a thick, firm cushion and to prevent movement. Seal the shipping container securely and mark it FRAGILE.

Preparation for Use
Packaging the Test Leads

3 Operation


Introduction

This Chapter describes using the test leads and compensation techniques for these test leads.

Test Leads Features

16089A/B/C

Figure 3-1 16089A/B/C Test Leads Features

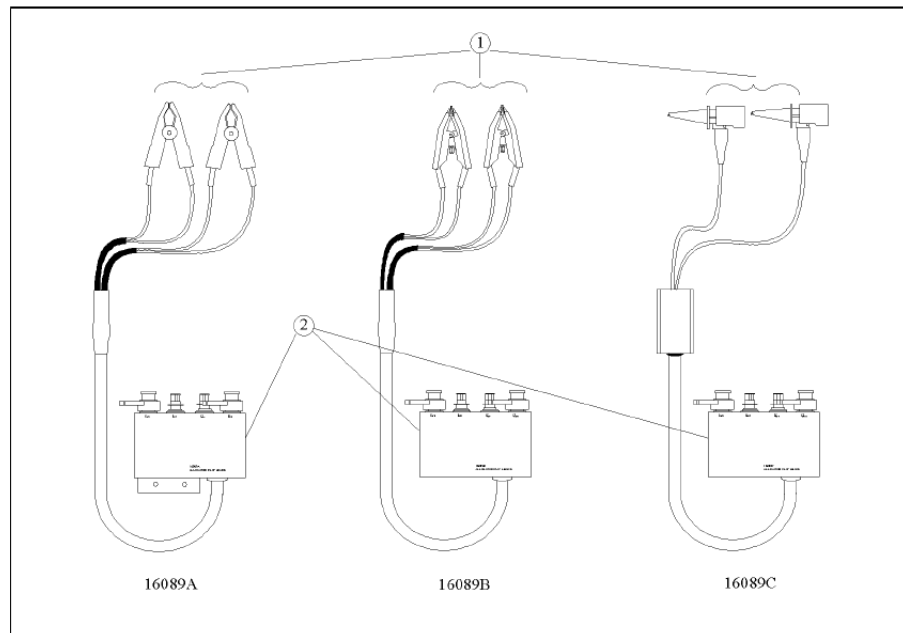


1. Kelvin Clips. These are connected to the DUT.
2. Four-terminal-pair BNC terminals. These terminals are connected to the UNKNOWN terminals of your measurement instrument.

OPEN and SHORT Compensation


The 16089A/B/C have inherent stray capacitance, residual inductance, and residual resistance that affect the measurement. To cancel the effects caused by these residuals and thus minimize their effect on measurement accuracy, the measurement instrument's OPEN and SHORT compensation capabilities must be used. The procedures are described in the measurement instrument's operation manual.

Figure 3-2 Making a Short Condition for the 16089B and 16089C

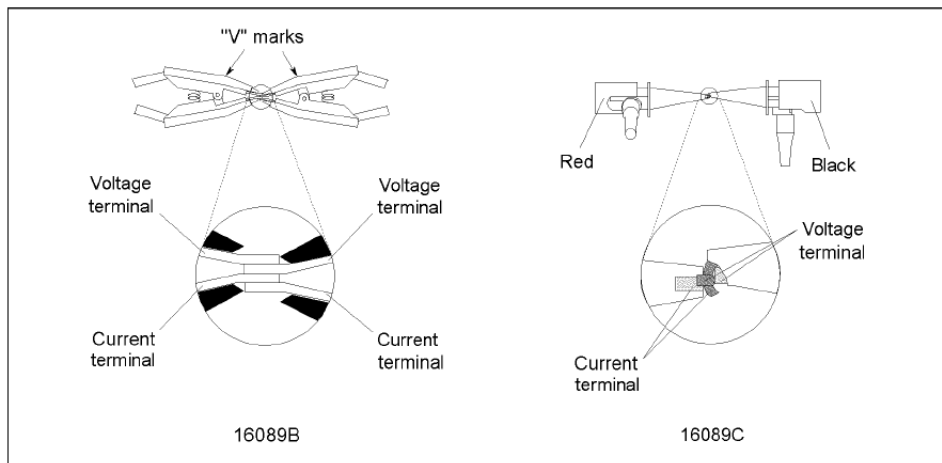

When you perform SHORT compensation for the 16089A, use the furnished short bar shown in [Figure 3-3](#).

Figure 3-3 Making a short Condition for the 16089A

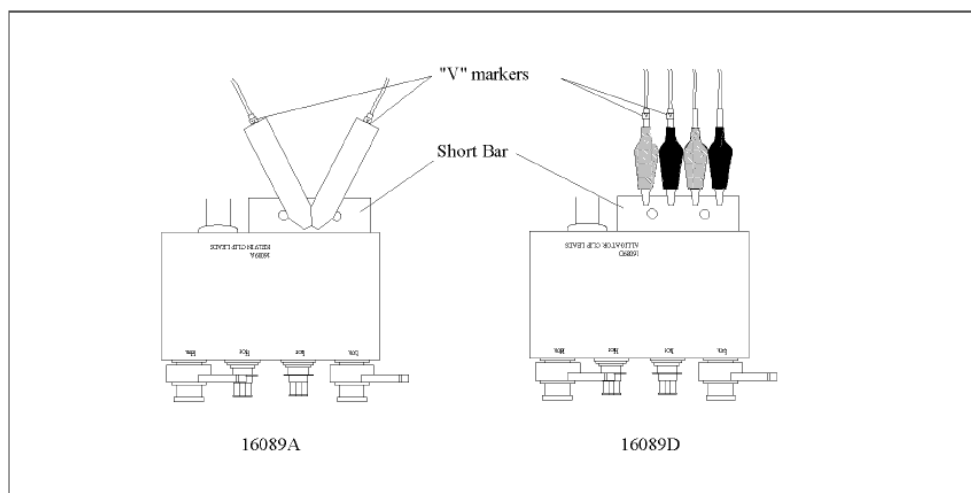

NOTE

If the furnished short bar of 16089A is corroded, worn or damaged, reverse the position or replace it with a new short bar. To reverse the short bar, remove the 2 screws that fixes the short bar and reverse the position.

Operation
OPEN and SHORT Compensation

Operation

Step-by-step instructions on how to make a measurement with the 16089A/B/C are:

1. Set the Cable Length setting according to the LCR meter/Impedance Analyzer operation manuals.
2. Connect the test leads of 16089A/B/C to the measurement instrument's UNKNOWN terminals.
3. Perform OPEN and SHORT compensation as described in the measurement instrument's operation manual. **Figure 3-2** and **Figure 3-3** show how to make short condition for the SHORT compensation.
4. Connect the component to be tested into the test clips.

Operation
OPEN and SHORT Compensation

4 Service

Introduction

This chapter gives replaceable parts information for the 16089A, 16089B and 16089C.

Serial Number for Non-RoHS Kelvin Clip Leads:

16089A: “MY44100001 – MY44199999” or “SG44100001 – SG44199999”

16089B: “MY40100001 – MY40199999” or “SG40100001 – SG40199999”

16089C: “MY44100001 – MY44199999” or “SG44100001 – SG44199999”

Serial Number for RoHS Kelvin Clip Leads:

16089A: “MY44200001 and above” or “SG44200001 and above”

16089B: “MY40200001 and above” or “SG40200001 and above”

16089C: “MY44200001 and above” or “SG44200001 and above”

Replaceable Parts

To order parts, use the Keysight part numbers listed in [Table 4-1](#), [Table 4-2](#) and [Table 4-3](#). If a faulty part is located in an assembly that cannot be disassembled, order the next higher assembly or return the fixture to the nearest Keysight Technologies Sales/Service Office for repair or replacement.

Shown are the supported parts and their respective RoHS compliant replacement support part. RoHS conversion involves with design and dimension change which result in the RoHS support part backward incompatible with non-RoHS test fixture. Special handling is needed while using the RoHS replacement part on non-RoHS test fixture. The original support part number is replaced by the respective “RoHS Compliant Replacement Part”. Once the original support part is depleted, please proceed to obtain the RoHS compliant support part.

16089A Replaceable Parts

Table 4-1

16089A Replaceable Parts

Keysight Non-RoHS Part Number	Description	Qty	RoHS Compliant Replacement Part	Description	Qty
16089-60001	Test Leads ¹	1	16089-60601 ²	Kelvin Clip Leads	1
16089-04001	Cover Top	1	16089-60601 ²	Kelvin Clip Leads	1
0515-0914	Screw Flat Head M3X0.5 L6	2	0515-1946	Screw Flat Head M3X0.5 L6	2
16089-60011	Large Clip Assembly	2	16089-60611	Large Clip Assembly	2
7121-2696	Wire Marker “V”	2	7121-2696	Wire Marker “V”	2
16089-01201	Short Bar	1	16089-01201	Short Bar	1
0515-1550	Screw	2	0515-0372	Screw	2

1. The whole unit. Keysight internal-only part.
2. For 2m test leads, please order 16089-60606 instead. (Both 16089-60606 and 16089-60601 are Keysight Internal part numbers only)

Red and orange cables are screwed on the one Kelvin clip assembly. Gray and black cables are screwed on the other Kelvin clip assembly. Orange and gray cables are marked “V”.

16089B Replaceable Parts

Table 4-2 16089B Replaceable Parts

Keysight Non-RoHS Part Number	Description	Qty	RoHS Compliant Replacement Part	Description	Qty
16089-60002	Test Leads ¹	1	16089B ²	Kelvin Clip Leads	1
16089-04002	Cover Top	1	16089B ²	Kelvin Clip Leads	1
0515-0914	Screw Flat Head M3X0.5 L6	2	0515-1946	Screw Flat Head M3X0.5 L6	2
16005-60010	Kelvin Clip Assembly	2	16005-60010	Kelvin Clip Assembly	2

1. The whole unit. Keysight internal-only part.
2. 16089-60602 is removed from support parts due to increasing costs. Purchase 16089B Medium Kelvin Clip Lead as the replacement.

On one Kelvin clip, the orange cable is screwed on the “V” marked side, and the red cable is screwed on the non-marked side. On the other Kelvin clip, the gray cable is screwed on the “V” marked side, and the black cable is screwed on the non-marked side.

16089C Replaceable Parts

Table 4-3 16089C Replaceable Parts


Ref /D ¹	Keysight Non-RoHS Part Number	Description	Qty	RoHS Compliant Replacement Part	Description	Qty
	16089-60003	Test Leads ²	1	16089-60603	Kelvin IC Clip Leads	1
	16089-04003	Cover Top	1	16089-60603 ³	Kelvin IC Clip Leads	1
	0515-0914	Screw Flat Head M3x0.5 L6	2	0515-1946	Screw Flat Head M3x0.5 L6	2
1	16005-60013	Test Clip Assembly Red	1	16005-60013	Test Clip Assembly Red	1
	16005-60015	Test Clip Assembly Black	1	16005-60015	Test Clip Assembly Black	1
2	0890-1809	Tube Heat Shrinkable Red	2cm	0890-2296	Tube Heat Shrinkable Red	2cm
	0890-1808	Tube Heat Shrinkable Black	2cm	0890-2295	Tube Heat Shrinkable Black	2cm

1. Corresponding to designator in **Figure 4-1**.
2. The whole unit. Keysight internal-only part.
3. Poka-Yoke Design Change. RoHS cover top (16089-04603) is not backward compatible with non-RoHS fixture. REplace the whole fixture.

Connection from the cables to the Kelvin clip is shown in **Figure 4-1**.

Figure 4-1

Kelvin Clip Connections

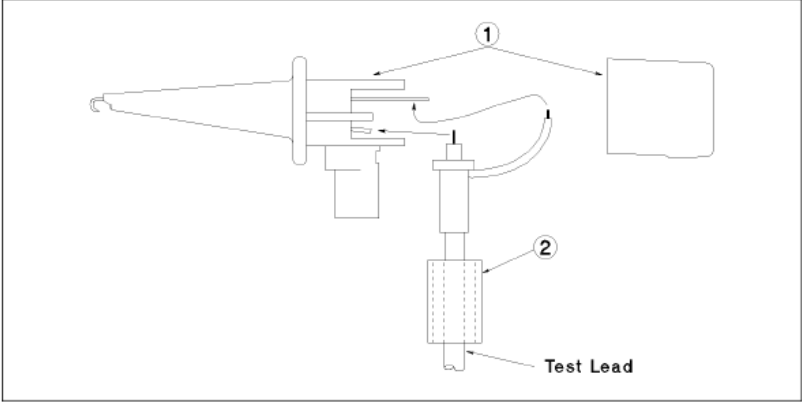

Service
Replaceable Parts

This information is subject to change without notice.
© Keysight Technologies 1999-2020
Edition 7, January 2020



16089-90030
www.keysight.com

X-ON Electronics

Largest Supplier of Electrical and Electronic Components

Click to view similar products for [Test Leads](#) category:

Click to view products by [Keysight](#) manufacturer:

Other Similar products are found below :

[795-2384-10-25](#) [1301430020](#) [1510-24-105](#) [15308](#) [15408](#) [15302](#) [15409](#) [BU-1149-A-36-0](#) [BU-1481-E-12-0](#) [BU-1481-E-24-0](#) [1927617](#) [2450](#)
[2524-A-60](#) [LB1F-2R-RED](#) [LB1F-2R-YLW](#) [2500](#) [2524-A-48](#) [2977-J-48](#) [R948131000](#) [380200](#) [BU-1449-E-12-2](#) [BU-1480-E-24-0](#) [BU-1481-](#)
[E-12-2](#) [BU-1481-E-24-2](#) [LB1F-2R-BLK](#) [LB1F-2R-BLUE](#) [LB1F-2R-WHT](#) [6345](#) [6432](#) [6416](#) [EM3782-24-3#](#) [R948161002](#) [R948160002](#)
[R948170002](#) [R948171002](#) [R948163002](#) [973604100](#) [934160101](#) [934160100](#) [R948174000](#) [CT3269](#) [CT3258](#) [CT3158-100](#) [HSPL](#)
[8568/AWG16/200/RT](#) [HSPL 8568/AWG16/200/SW](#) [28.0119-10020](#) [28.0127-05025](#) [28.0127-20025](#) [49.0079-20021](#) [49.0079-20024](#)